



Aerosol Therapy

Model #: _____
Serial #: _____
Date: _____


Provider Name: _____
Phone #: _____
Contact Person: _____

Setting up your equipment:

- Place aerosol compressor on a solid, flat surface
- Assemble nebulizer kit
- Attach tubing to compressor outlet and to nebulizer
- Place medication into nebulizer medicine cup
- Place 'T' with mouthpiece onto nebulizer

Frequent replacement items:

- Nebulizer kit approximately every 2 weeks
- Compressor filters

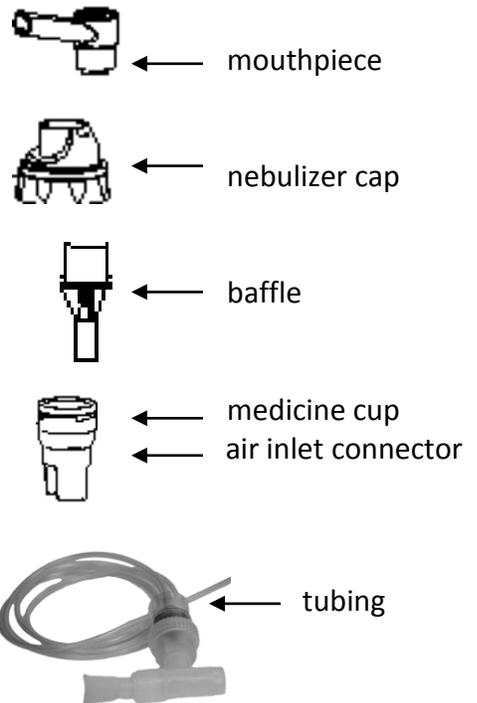

Using your equipment:

1. Plug aerosol into grounded outlet. Make sure power on compressor is in the "OFF" position.
2. Add medication to nebulizer and connect tubing to the compressor air outlet.
3. Switch the compressor "ON"; the medication will begin to 'mist'.
4. Breath slowly and deeply; holding the mist in your lungs every few minutes. Continue until medication is gone.
5. Once completed, switch "OFF" the compressor and disassemble nebulizer.



Special Procedures:


- If using a portable nebulizer, refer to “Using Your Equipment” for treatment procedure.

Safety Issues:

- Check with physician for any drug sensitivity and ensure medication is compatible with all other current medications you may be taking.
- Should your pulse increase by more than 30 BPM, discontinue treatment & consult physician.
- You may experience shakiness during the treatment. Should this occur, discontinue treatment. Resume after a few minutes. If this sensation persists, consult your physician.
- Check expiration on medication, and do not use if medication is expired.

Maintenance:

- Rinse nebulizer after every treatment and place on dry paper towel. At end of the day, wash all of the parts with warm soapy water, rinse and soak with 1:3 vinegar and water solution for 30 minutes and rinse.
- Your local provider may recommend a germicidal disinfectant solution to clean your nebulizer rather than vinegar and water. Mix with water according to directions, and you can store it for up to 30 days. Always rinse your equipment after cleaning.
- Replace compressor filters whenever material becomes discolored.

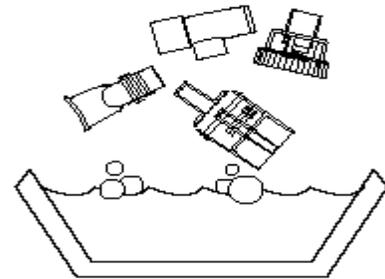

Please contact your equipment provider for any questions, adjustments, or repairs.

Your Local Provider:



©Copyright The VGM Group
B.L.U.E. Sheet images, drawings, and text
courtesy of VGM contracted vendors.

All Medicare DMEPOS suppliers must be in compliance with CMS Supplier Standards in order to obtain and retain their billing privileges. These standards, in their entirety, are listed in 42 C.F.R. pt. 424, sec 424.57(c). A supplier must disclose these standards to all customers/patients who are Medicare beneficiaries (standard 16). Supplier Standard 12 includes “A supplier ...must instruct beneficiaries on use of Medicare covered items”.